Getting to know the quick select buttons

Using the quick select buttons, the set functions are called up directly. Factory settings:

> Left quick select button ①: Adjust scaling.
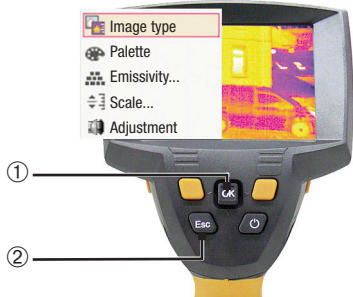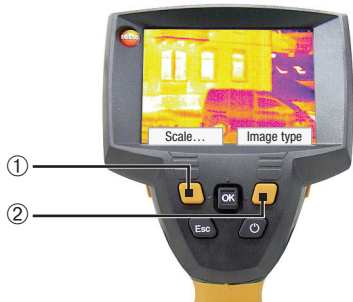> Right quick select button ②: Select image type.

⚠ **Warning!** Eye damage due to laser beam.

> Do not look into the laser beam and do not point the laser beam at people.

Changing assignment of the quick select buttons

Change the left or right quick select button:

1 Call up: Move **Joystick** ① to the left or right.
2 Navigate: Move **Joystick** up / down.
3 Confirm: Press **[OK]** ①.
   or
   Cancel: Press **[Esc]** ②.

testo 875i · Thermal imager

Brief instructions   en

Building inspection

Electrical maintenance work

Mechanical maintenance

Contact

GREAT BRITAIN / IRELAND
Testo Ltd.
Alton, Hampshire GU34 2QJ
Tel. (14 20) 54 44 33, Fax (14 20) 54 44
E-mail: info@testo.co.uk

USA
Testo Inc.
Flanders, NJ. 07836
Tel. (973) 2 52 17 20, Fax (973) 2 52 17 29
E-mail: info@testo.com

AUSTRALIA
Testo Pty Ltd
Croydon South VIC 3136
Tel. (3) 98 00 46 77, Fax (3) 98 00 46 99
E-mail: info@testo.com.au

The most up-to-date address details of our subsidiaries and agencies can be found in Internet at: www.testo.com
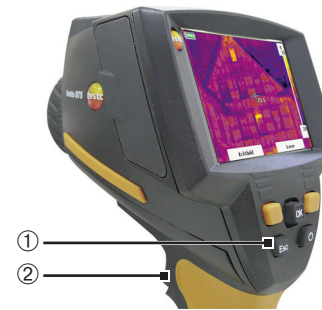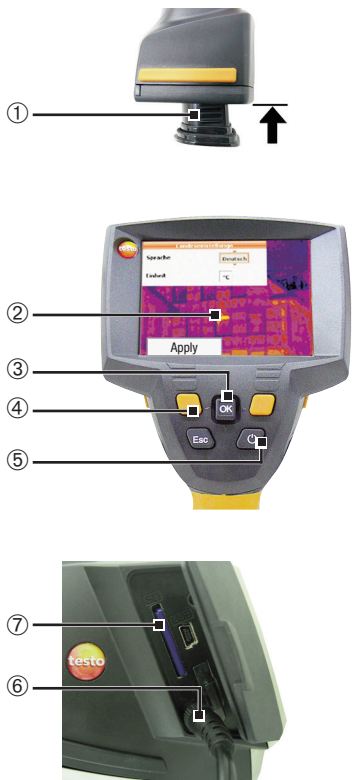
Commissioning

1 Push the **rechargeable battery** ① all the way into the rechargeable battery slot until this is flush with the bottom of the handle.

- The thermal imager starts automatically.

2 Remove protective film from the **display** ②.

- Instrument language (**Language**) and temperature unit (**Unit**) can be set:

3 Move **Joystick** ③ up / down to select the desired option.

4 Press **[OK]** ③.

5 Move **Joystick** up / down to change the setting.

6 Press **[OK]**.

7 Press **[Apply]** ④ function key to apply the settings.

8 Press **[⏻]** ⑤ to switch off the thermal imager.

9 Connect **mains unit** (🔌) ⑥.

10 Completely charge battery (3 hours).

11 Insert **Memory card** in the card slot (**SD**) ⑦.

- The camera is now ready for operation.

Switching on / off

➤ Remove **protection cap** ① from the lens.

➤ Switch on: Press **[⏻]** ②.

- The measurement view is opened after the warm-up period.

- The thermal imager performs an automatic zeroing approx. every 60 sec. This can be recognized by a "click". The image is frozen briefly when this occurs.

➤ Switch off: Press **[⏻]** again.

Focusing the picture

➤ Turn **lens** ① by hand.

Recording the image

1 Freeze image: Press trigger button ② once.

2 Save image: Press trigger button again.
or
Discard image: Press **[Esc]** ①.

Getting to know the menu

1 Open menu: Press **[OK]** ①.

2 Navigate: Move **Joystick** ① up / down.

3 Open submenu (only for menu points marked with ▶): Move joystick to the right.

4 Call up a function: Press **[OK]**.
or
Exit menu: Press **[Esc]** ②.